

# VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

APR 01 2011

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: 130193

Supervisor/Operator Performing the Verification Procedure:

Name: JAMES C. GIPSON ID#: 4842 Date: 18 March 11

A

Agency: Palmer Police Department Phone #: (907) 745-4811

Instrument Location: Palmer Police Department

B

Alco S/N: 77199 Target Value: .078 High Pressure: 600

Alco Test Value Average: .079 .079  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco


Signature: \_\_\_\_\_

(OVER)


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

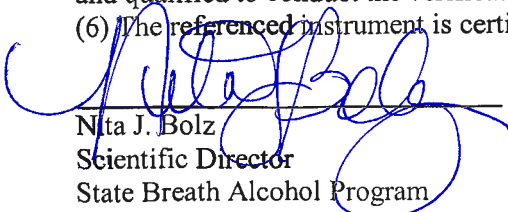  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 1<sup>st</sup> day of APRIL, 2011

  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

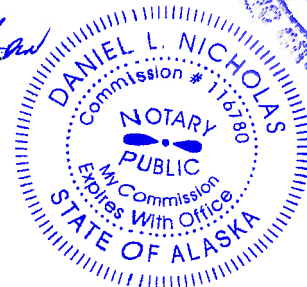

# VERIFICATION OF CALIBRATION REPORT

*Of DataMaster cdm Breath test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program*

DataMaster cdm S/N: 130193

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

MARCH 18, 2011

OPERATOR'S NAME: *BMB 4/11/11*  
GIPSON/JAMES/C  
OPERATOR'S NUMBER: 4842  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
RJCSB  
O.L. #: 0123456  
DEPT/AGENCY: PLM1  
CASE/REPORT: 01-2345  
TEST TYPE: U  
ALCO TARGET VALUE: .078  
ALCO S/N: 77199

— BREATH ANALYSIS —

.078 ADJUSTED FOR 30.11 in		
ALCO TARGET	.078	14:00
BLANK TEST	.000	14:01
INTERNAL STANDARD	VERIFIED	14:01
ALCO TV 30.11 in	.079	14:01
BLANK TEST	.000	14:02
SUBJECT SAMPLE	.000	14:04
BLANK TEST	.000	14:05
ALCO TV 30.12 in	.079	14:05
BLANK TEST	.000	14:06

*BMB 4/11/11*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

MARCH 18, 2011  
TIME 13:53

— DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	41c
BAROMETER:	30.12 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMNPOQRSTUVWXYZ[\]^\_`'abcdefgijklmno  
pqrstuvwxyz{|}~